


# MEDITECH Expanse TIP SHEET

## Hemodialysis Settings Enhancement

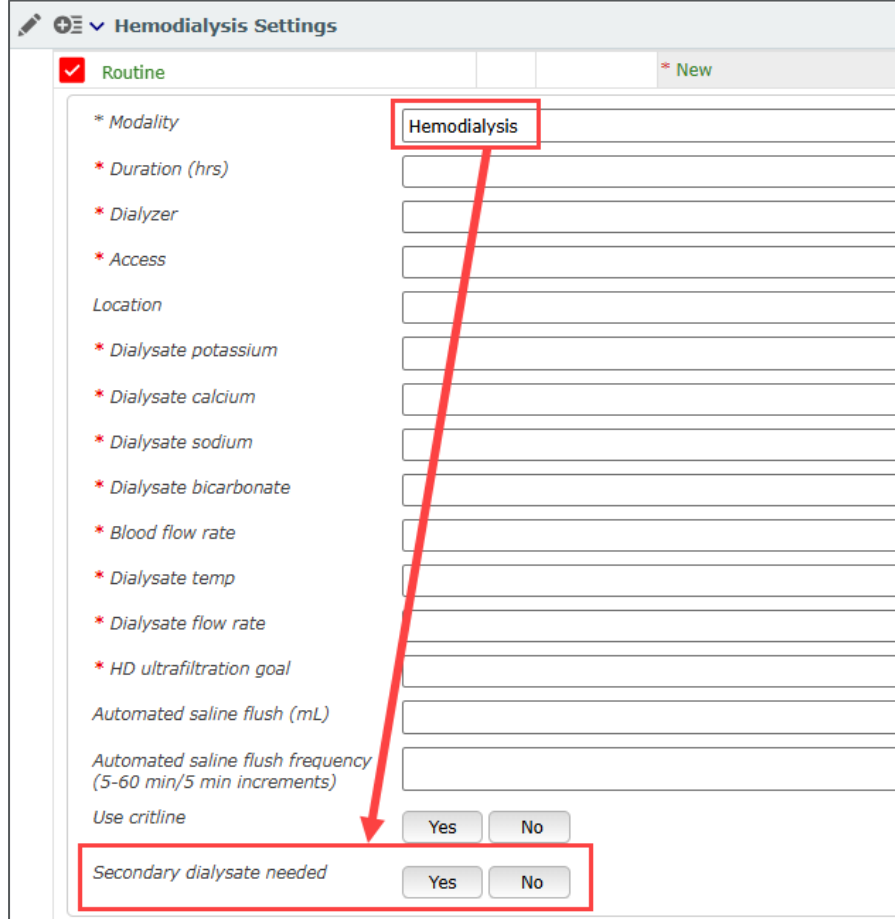

**Hemodialysis Settings**

☒ Routine \* New

\* Modality Hemodialysis

\* Duration (hrs)

\* Dialyzer

\* Access

Location

\* Dialysate potassium

\* Dialysate calcium

\* Dialysate sodium

\* Dialysate bicarbonate

\* Blood flow rate

\* Dialysate temp

\* Dialysate flow rate

\* HD ultrafiltration goal

Automated saline flush (mL)


Automated saline flush frequency (5-60 min/5 min increments)

Use critline


Secondary dialysate needed

Within the Hemodialysis Settings order, when a modality of *Hemodialysis* is selected, users will have a new optional query available titled:

- Secondary dialysate needed

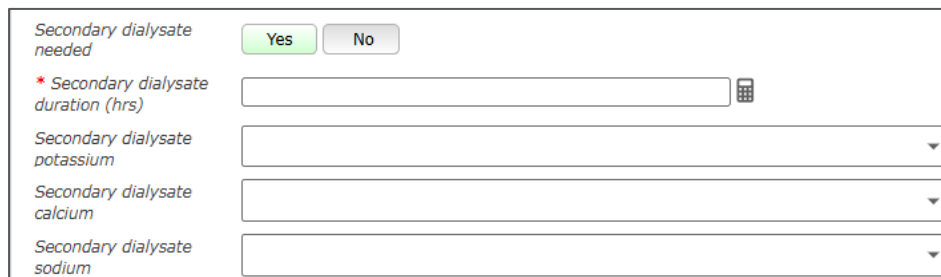

Secondary dialysate needed

\* Secondary dialysate duration (hrs)  

Secondary dialysate potassium

Secondary dialysate calcium

Secondary dialysate sodium

If a user indicates that a secondary dialysate is needed, they are required to designate the:

- Secondary dialysate duration (hrs)

They also have the option to designate:

- Secondary dialysate potassium
- Secondary dialysate calcium
- Secondary dialysate sodium